High - Low Exam Table Installation

[Refer to User's Guide for description of safety symbols]

Applies to Models

222 (all)
223 (all)
622 (all)
623 (all)

Equipment Alert

Failure to follow these instructions may result in damage to the table.

NEVER push on base covers.

NEVER use stirrups to lift table.

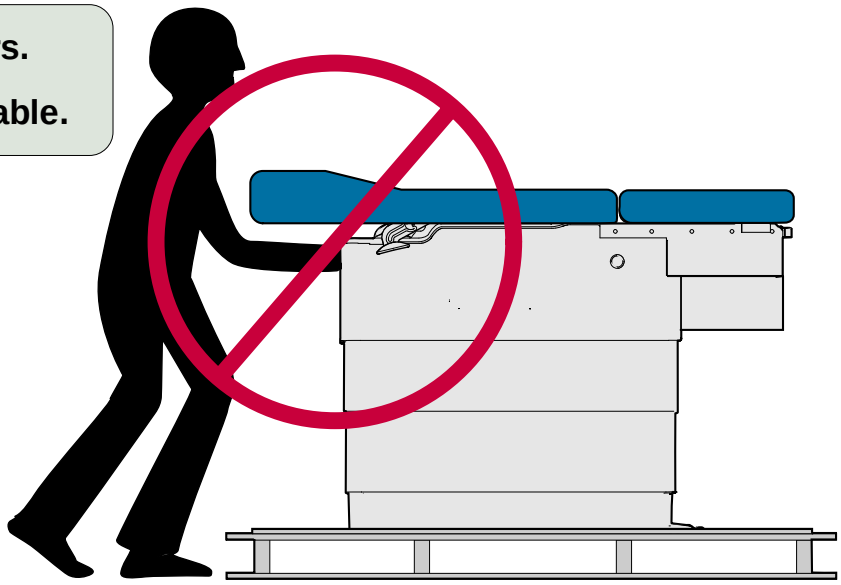

ALWAYS transport table in "full-down" position.

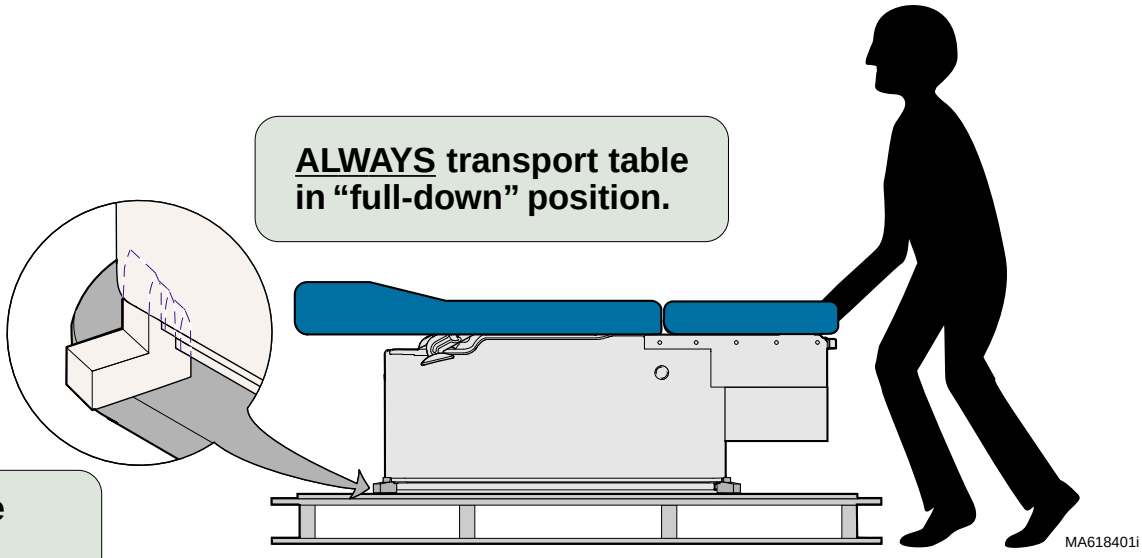

ALWAYS leave (4) base cover supports in place until final delivery.

© Midmark Corporation 2003

003-1359-00 Rev. (A)

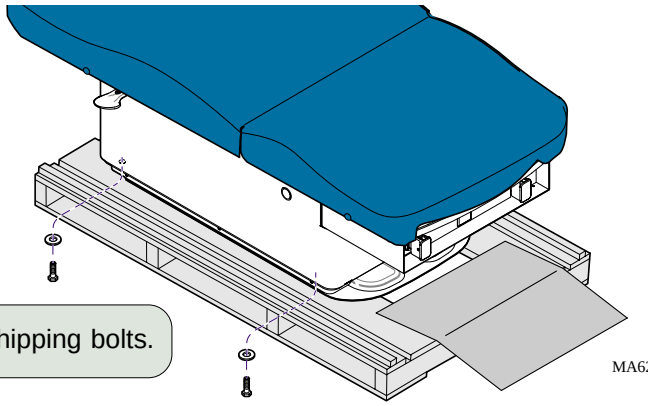

Step 1: Remove shipping bolts.

MA622700i

Equipment Alert

Table must be leveled to ensure proper operation.



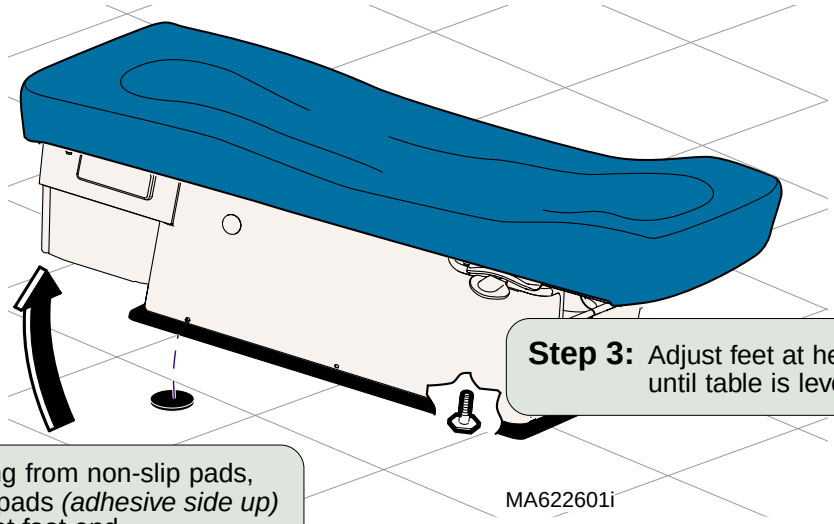

Step 3: Adjust feet at head end until table is level.

Step 2: Peel backing from non-slip pads, then place pads *(adhesive side up)* under feet at foot end.

MA622601i

Electrical Ratings

Models: 222, 223, & 622 (115 VAC)
Dedicated Supply Circuit: 115 VAC, 50/60 Hz, 15 Amp

Model: 623 (115 VAC)
Dedicated Supply Circuit: 115 VAC, 50/60 Hz, 20 Amp

Models: 222, or 223 Series (230 VAC)
Dedicated Supply Circuit: 230VAC, 50/60 Hz, 15 Amp

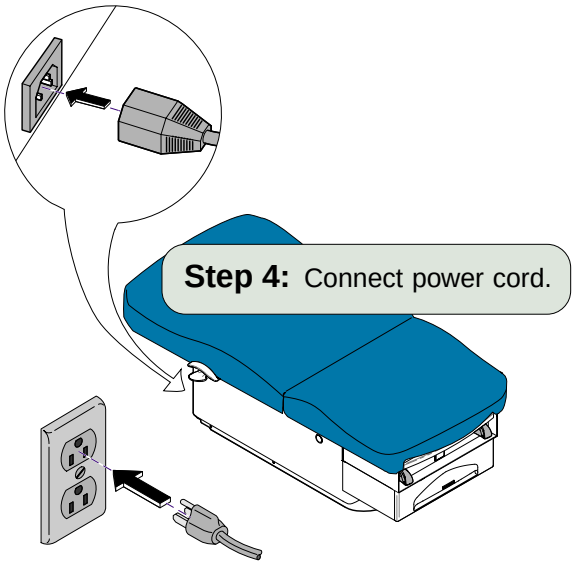

Step 4: Connect power cord.

MA600101i

Note

This step applies to 223 & 623 models only.

Step 5: Connect foot control.
223: *foot end.*
623: *foot or head end*

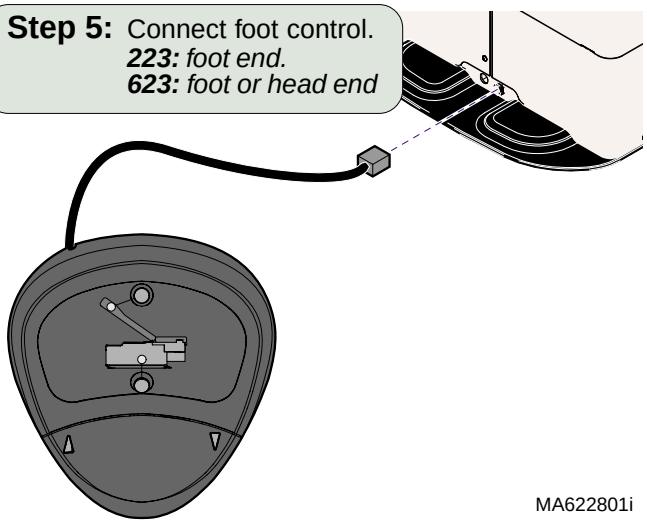

MA622801i

© Midmark Corporation 2003